

FIG. 2

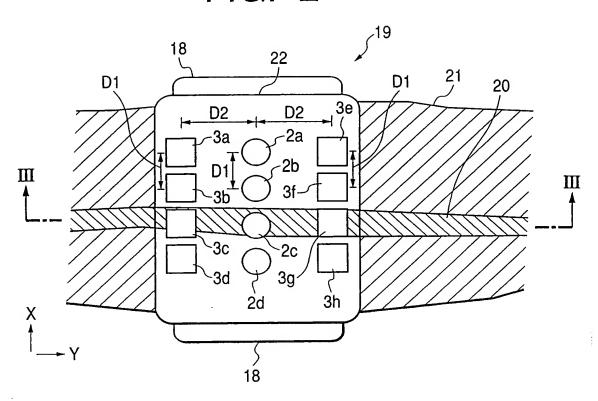
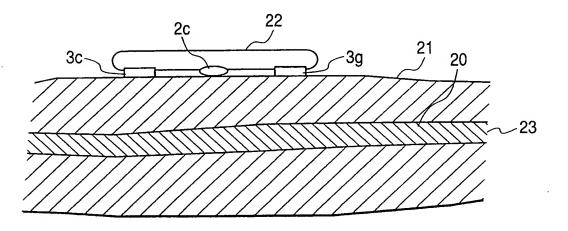


FIG. 3



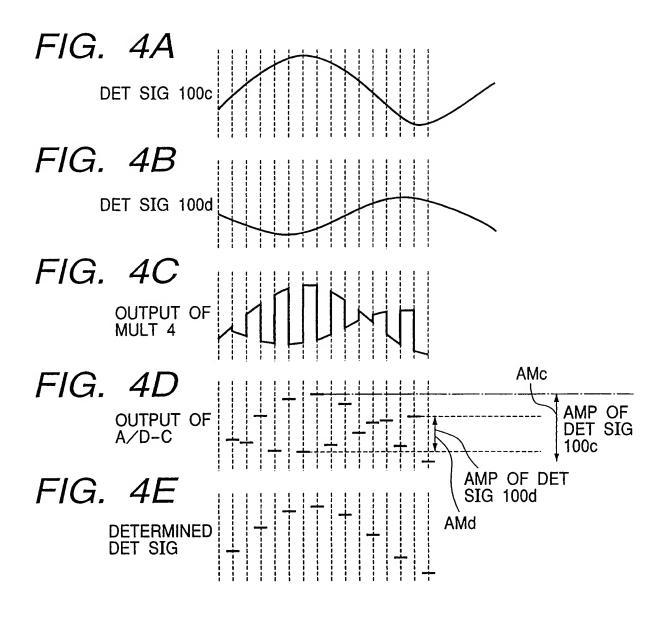


FIG. 5A

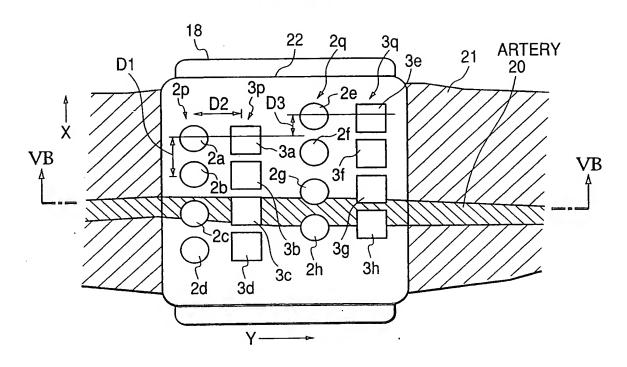
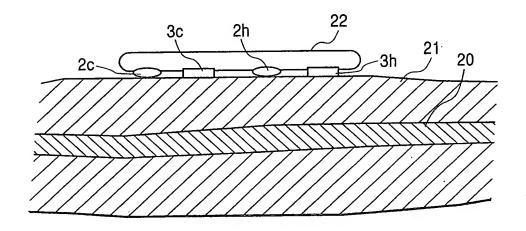
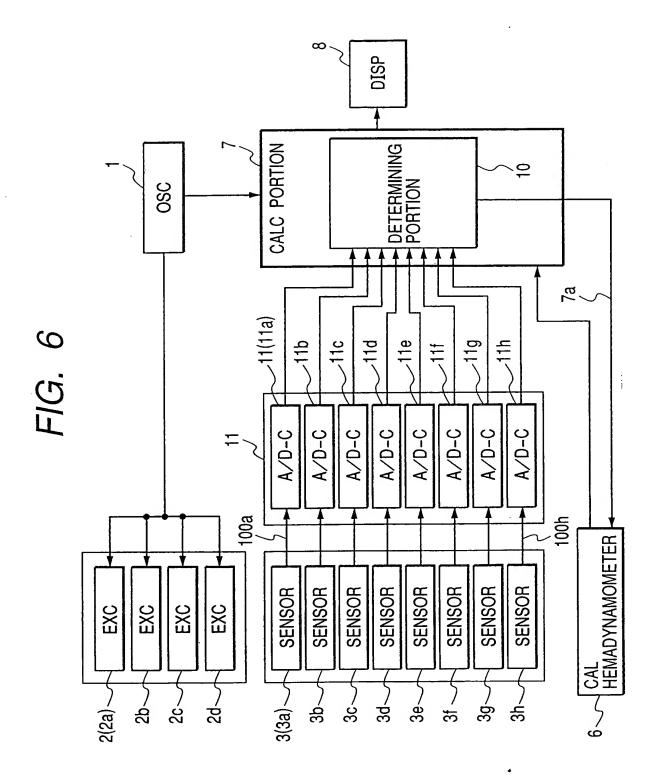
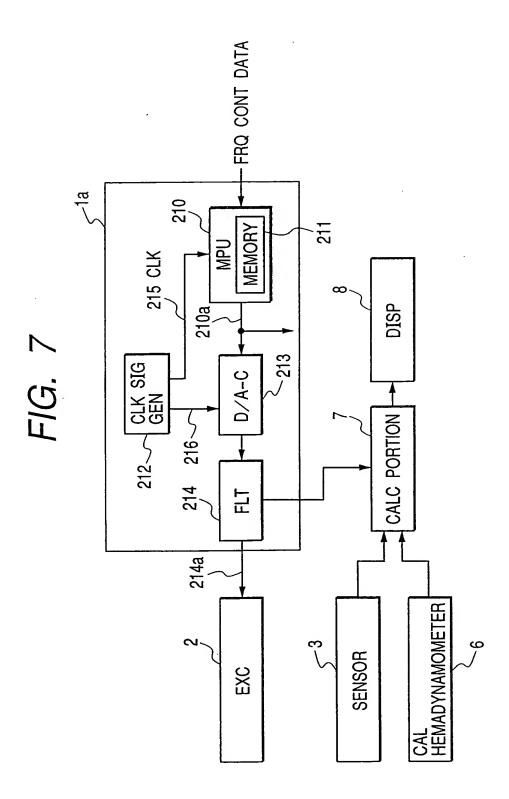


FIG. 5B







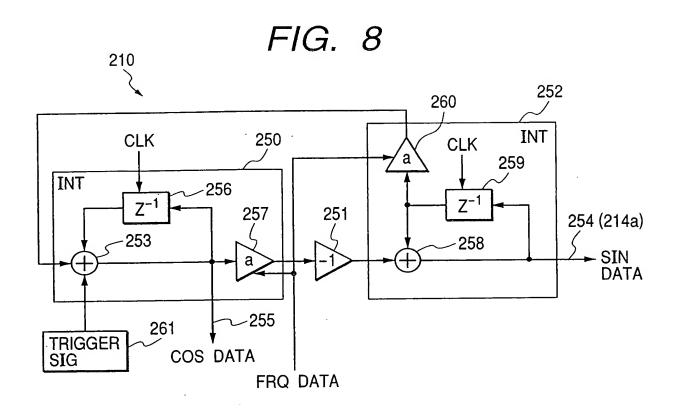


FIG. 9 -1b 222 CLK SIG GEN 224 223 220 CLK 221-NUMERICAL-CONTROLLED OSC FRQ CONT DATA **EXC SENSOR** CALC PORTION DISP **HEMADYNAMOMETER** -6



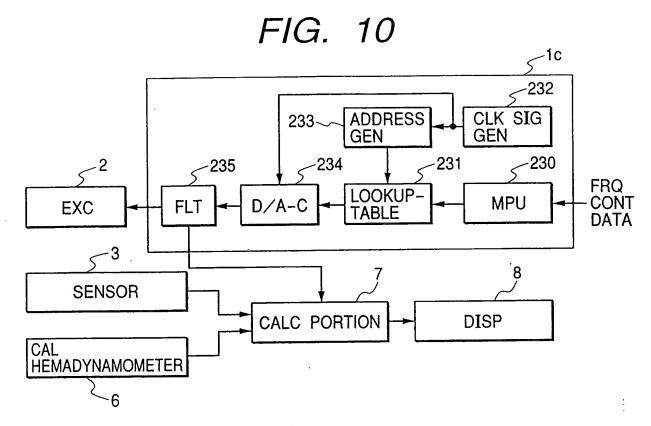


FIG. 11

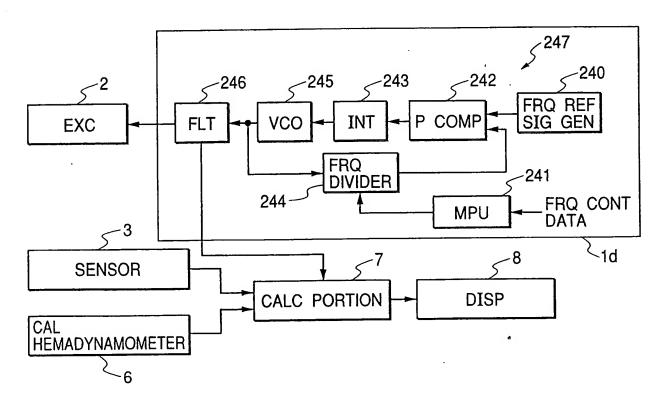


FIG. 12

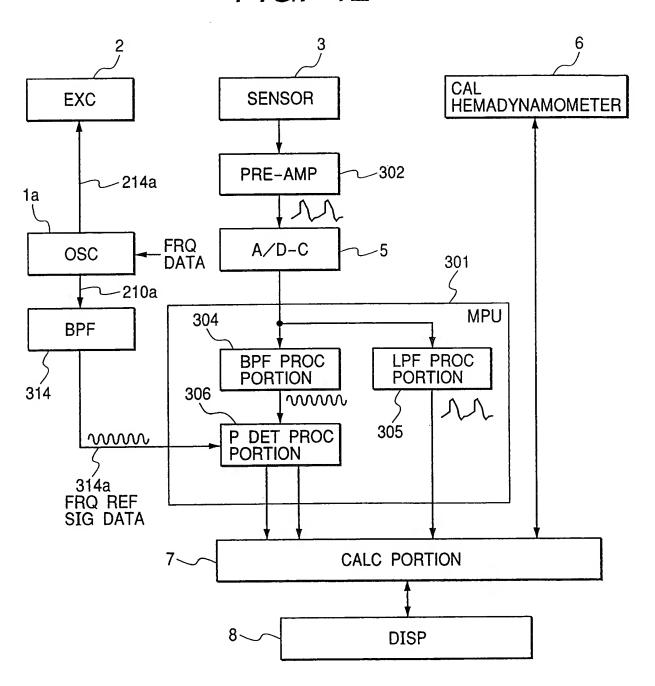


FIG. 13A

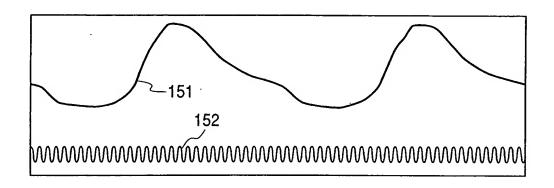


FIG. 13B

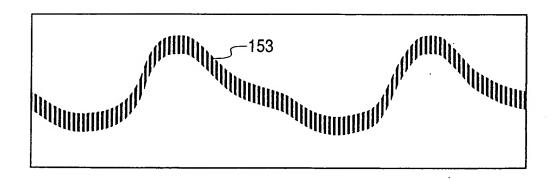
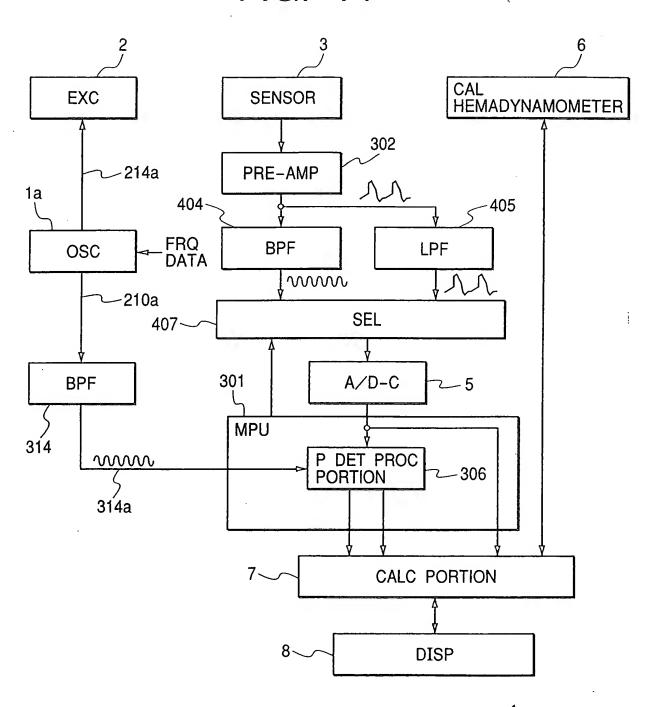


FIG. 14



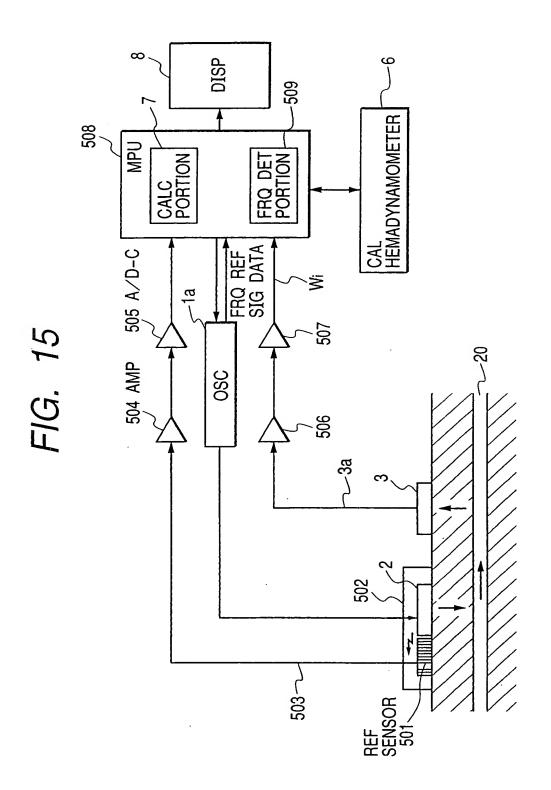


FIG. 16



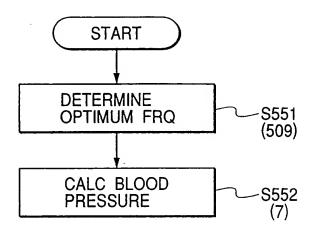


FIG. 18

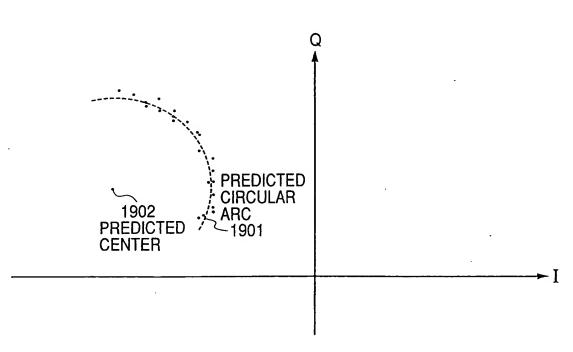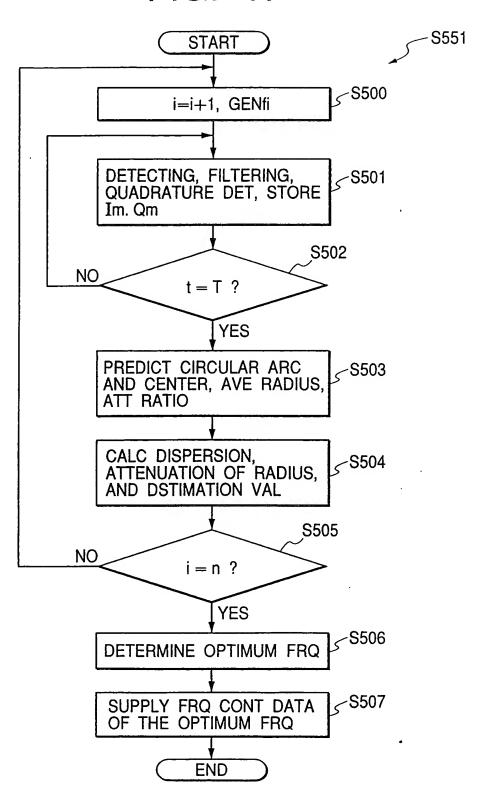

1

FIG. 17



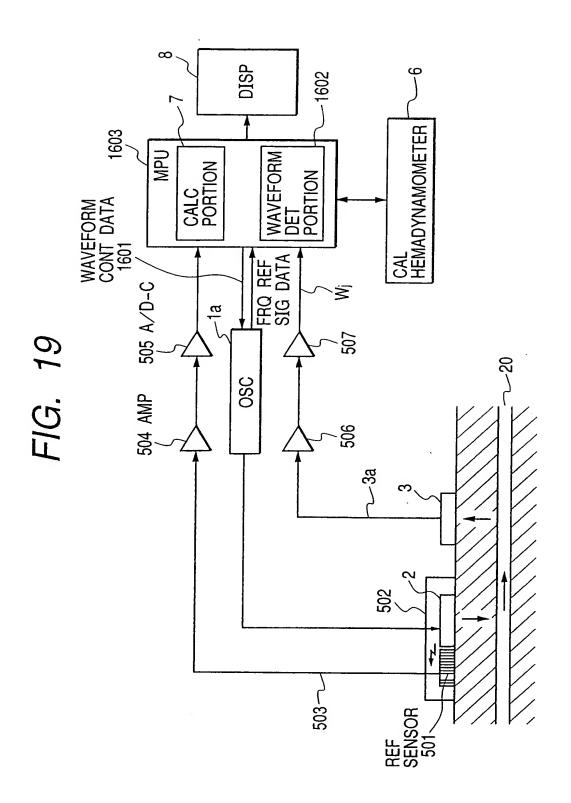


FIG. 20

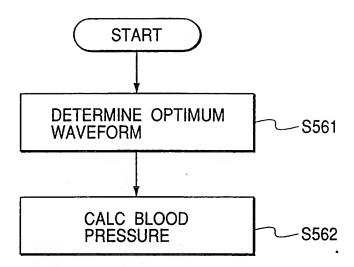


FIG. 21

